

# Comparative Evaluation of Nanoscale Surface Coatings on Silicon Substrates for Implantable Device Applications

Zohora Iqbal,<sup>1</sup> Brooke Benner,<sup>1</sup> Charles Blaha,<sup>1</sup> Jaehyun Park,<sup>1</sup> Eun Jung Kim,<sup>1</sup> Steven Kim,<sup>2</sup> William H. Fissell,<sup>3</sup> Shuvo Roy.<sup>1</sup>

<sup>1</sup>Bioengineering, UCSF

<sup>2</sup>Nephrology, UCSF

<sup>3</sup>Nephrology, Vanderbilt University

## Background:


Highly uniform silicon nanopore membranes (SNM) are under investigation for use in implantable devices for organ replacement functions. A robust, readily scalable, non-fouling surface coating is required to enhance SNM biocompatibility while preventing pore occlusion. We evaluated a number of thin-film surface coatings compatible with silicon processing techniques. Five candidate biocompatible coatings were optimized for sub-5 nm deposition and evaluated for protein resistance.

## Methods:


Silicon surfaces were modified using 1) surface grafted self-assembled monolayer polyethylene glycol (PEG); 2) RF plasma polymerized PEG; 3) poly(sulfobetaine methacrylate) (pSBMA) grown on surface via atom-transfer radical polymerization (ATRP); 4) poly(2-methacryloyloxyethyl phosphorylcholine) (pMPC) coated via ATRP; and 5) titanium oxide (TiO<sub>2</sub>) deposited via atomic layer deposition. Coating thickness was determined by ellipsometry. Protein adsorption was determined by enzyme-linked immunosorbent assays after 2-hour incubation in single protein solutions of human fibrinogen and albumin. All adsorption data was normalized to uncoated silicon substrates.

## Results:

Average coating thickness for the coatings ranges between 0.7 nm to 4.7 nm (Figure 1). All coatings exhibited reduced protein adsorption compared to non-coated substrates (Figure 2). TiO<sub>2</sub>-coated silicon had the highest overall fouling, while pSBMA exhibited least fouling with an 84% reduction in human albumin adsorption and 98% reduction in human fibrinogen adsorption compared to bare silicon. The results demonstrate that pSBMA-coated surface exhibit superior non-fouling characteristics that make it suitable for application to SNM-based devices.

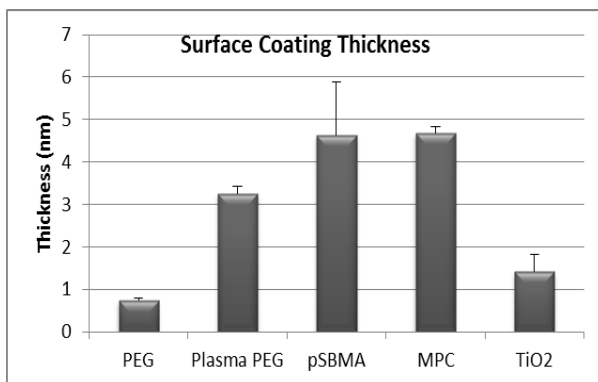

**Figure 1:** Surface modification coating thickness.

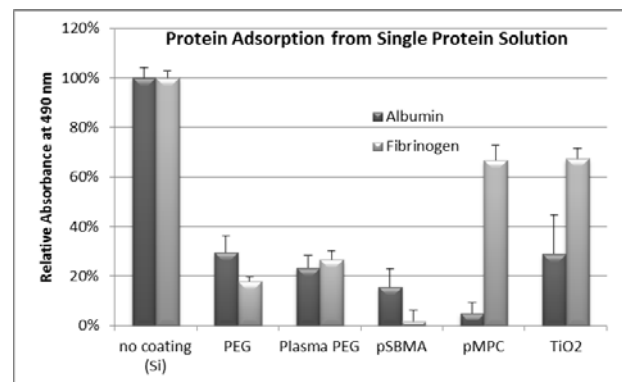

**Figure 2:** Normalized protein adsorption of human albumin and fibrinogen from single protein solutions.